

# TB750G

Right Angle Scattered Light Turbidimeter

# Yokogawa Next Generation Turbidimeter TB750G

Since their sales began in 1959, Yokogawa's turbidimeters have been continuously developed and improved using various measurement principles suited for various applications. With its many achievements, Yokogawa has earned its customers' confidence.


Developed based on years of experience and applications in process fields, the TB750G Turbidity Measuring System using right angle light scattering method provides highly reliable measurement and improved maintainability which improve upon what previous models could offer. A wide range of options are available to meet users' various needs.

## FEATURES

- **Easy-to-clean cell**
- **Bubble trap structure cell**
- **Ultrasonic cleaning**
  - Ultrasonic transducer and oscillator for ultrasonic cleaning (Optional)
- **In-line connection available**
  - Detector can be also connected for in-line analysis
- **Highly reliable measurement with excellent linearity and repeatability**
  - Linearity:  $\pm 2\%$  of reading or  $\pm 0.01$  NTU, whichever is greater
  - Repeatability:  $\pm 1\%$  of reading or  $\pm 0.002$  NTU, whichever is greater
- **User configurable measuring range**
  - Measuring range: 0-0.2 NTU to 0-100 NTU
- **A wide range of measurement conditions**
  - Low flow rate: 0.05 to 20 L/min
  - High pressure: 500 kPa maximum
  - Temperature: 0 to 50°C
- **Others**
  - Measuring range switching (2 or 3 ranges)
  - Enhanced self-diagnostic function as standard
    - Light source failure, input element failure, calibration failure, various circuit failures, etc.
  - 2 analog outputs, 3 relay contact outputs, and 1 digital output
  - Various head tanks to accommodate application requirements (Optional)
  - Compact, lightweight converter and detector




## DETECTOR

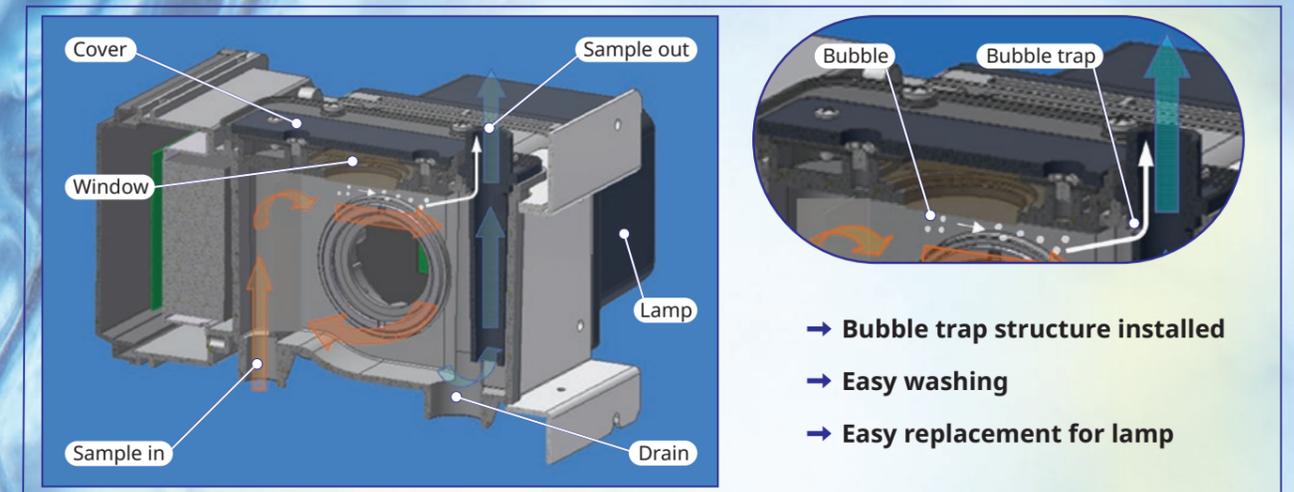

- Bubble trap structure installed
- Easy washing
- Easy replacement for lamp


## CONVERTER

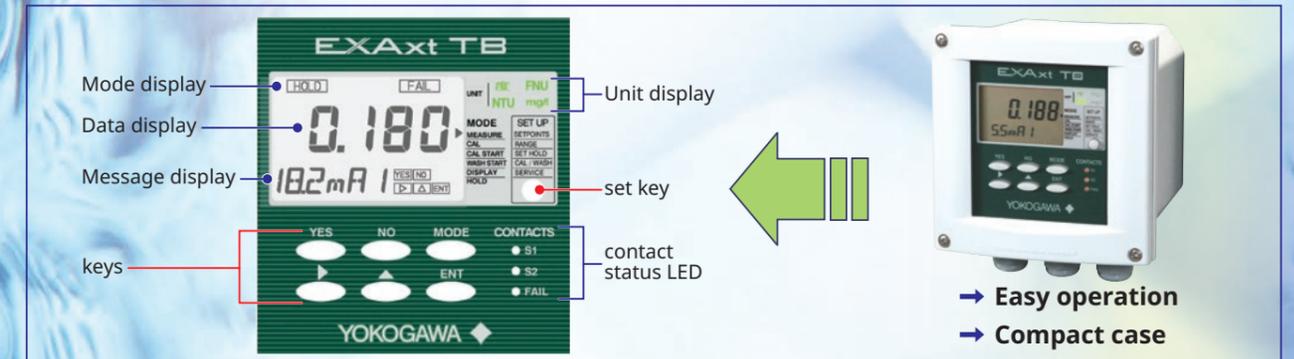


- Easy operation
- Compact case

## SYSTEM CONFIGURATION

### Typical system

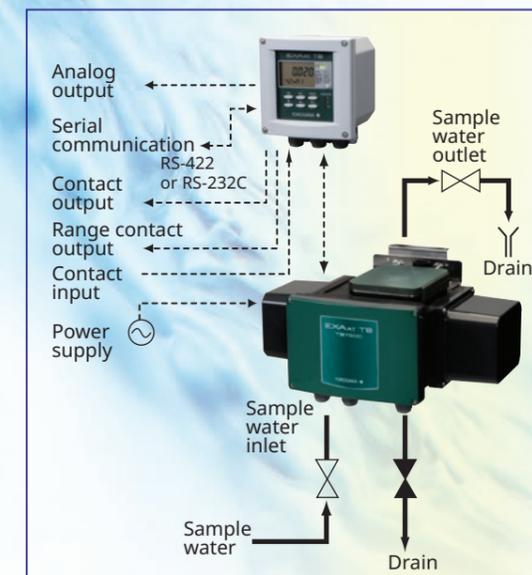

### System with ultrasonic oscillator and zero turbidity filter

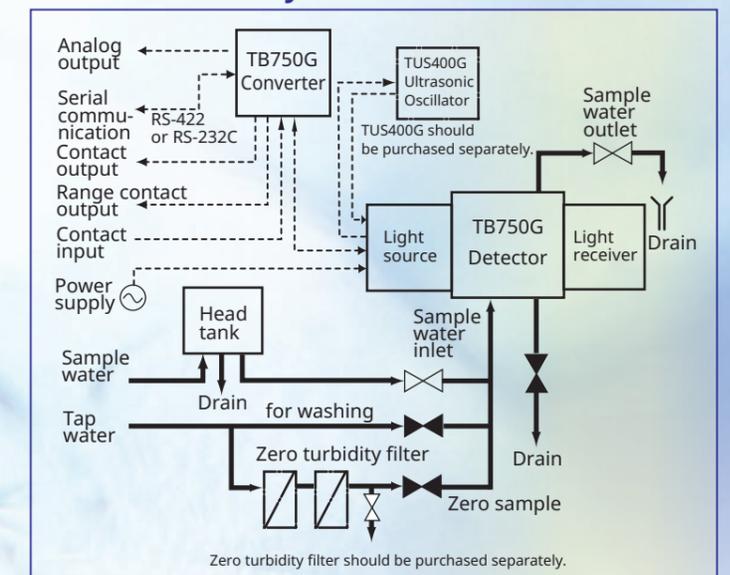


## SPECIFICATIONS

Measurement	Turbidity of finished water and water used in general processes
Measuring range	0.000 to 100.0 NTU
Display resolution	0.001 NTU
Output signal	Analog output 1; 4 to 20 mA DC, isolated Analog output 2; 4 to 20 mA DC or 0 to 20 mA DC selectable, isolated Load resistance; 550 Ω max.
Output range	Configurable within the measuring range Minimum range; 0 to 0.2 NTU Maximum range; 0 to 100 NTU Minimum span; 20% or more of upper limit of the range or 0.2 NTU, whichever is greater
Serial communication	RS-422 or RS-232C, isolated
Contact output	3 relay contact outputs
Contact input	2 contacts
Range contact output	3 relay contact outputs
Ambient temperature	-5 to 50°C (Sample and tap water may need protection against freezing)
Ambient humidity	5 to 95%RH (non-condensing)
Power supply	100 to 240 VAC -15%/+10%, 50/60 Hz
Power consumption	Converter+Detector; 50 VA max.
Sample water conditions	Flow rate: 0.05 to 20 L/min, Pressure: 500 kPa max., Temperature: 0 to 50°C
Mounting	Pipe, wall, rack or panel mounting
Standard performance	Repeatability: ±1% of reading or ±0.002 NTU, whichever is greater Linearity: ±2% of reading or ±0.01 NTU, whichever is greater Response time: Within 2 minutes (90% response, sample water flow rate 3 L/min)
Weight	Detector; Approx. 5.8 kg, Converter; Approx. 1.5 kg


\*Refer to GS 12E01A06-01E for details.

## EXTERNAL DIMENSIONS

### Converter

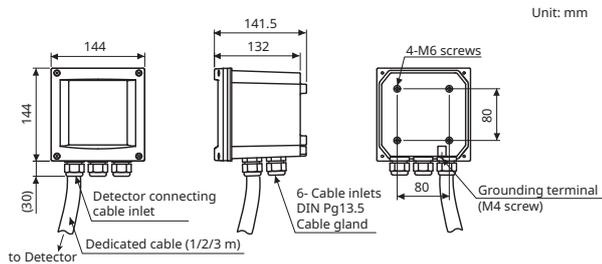

### Detector

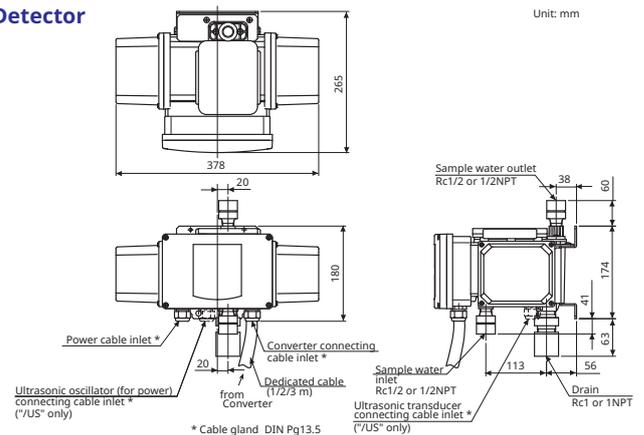

## MODEL AND CODES

**TB750G Right Angle Scattered Light Turbidimeter** [Style : S1]

Model	Suffix Codes	Option Codes	Description
TB750G	.....	.....	Right angle scattered light turbidimeter
Turbidity standard and measuring range	-NTU	.....	Formazine, 0-0.2 NTU to 0-100 NTU
Application	-ST	.....	Standard
Output	-N1 -N2	..... .....	4 to 20 mA DC, RS-422 4 to 20 mA DC, RS-232C
Sampling system	-NN	.....	Without sampling system
Sampling system material and mounting	NN	.....	Without sampling system
Cable length between converter and detector	-1 -2 -3	..... ..... .....	1 m 2 m 3 m
-	-NN	.....	Always -NN
Option	Detector process connection Mounting hardware	/NPT /U /R  /PM /TBC	ANSI standard connection Pipe mounting hardware (SUS) Rack or wall mounting hardware (SUS) Panel mounting hardware (SUS) Mounting hardware for Model 8562 or Model TB500G replacement (SUS)
	Conduit adapter	/AFTG /ANSI	G1/2 1/2NPT
	Head tank	/D1 /D2	Pressurized head tank for low turbidity (recommended for 2.0 NTU or less) Simple head tank
	Tag plate	/SCT	Stainless steel tag plate
	Special painting	/X1	Epoxy painting
	Ultrasonic transducer	/US	Transducer for ultrasonic cleaning

Note: When ultrasonic cleaning is continuously used after the Model 8562 Turbidity Transmitter has been replaced with the TB750G Turbidimeter, this "/US" option must be specified.

### Trademarks

All brand or product names of Yokogawa Electric Corporation in this document are trademarks or registered trademarks of Yokogawa Electric Corporation. All other company brand or product names in this bulletin are trademarks or registered trademarks of their respective holders.

### YOKOGAWA ELECTRIC CORPORATION

#### World Headquarters

9-32, Nakacho 2-chome, Musashino-shi, Tokyo 180-8750, JAPAN

<http://www.yokogawa.com/an/>

### YOKOGAWA CORPORATION OF AMERICA

#### YOKOGAWA EUROPE B.V.

#### YOKOGAWA ENGINEERING ASIA PTE. LTD.

#### YOKOGAWA CHINA CO., LTD.

#### YOKOGAWA MIDDLE EAST & AFRICA B.S.C.(c)

<http://www.yokogawa.com/us/>

<http://www.yokogawa.com/eu/>

<http://www.yokogawa.com/sg/>

<http://www.yokogawa.com/cn/>

<http://www.yokogawa.com/bh/>

Represented by:

ANA-01E

Subject to change without notice.

All Rights Reserved, Copyright © 2005, Yokogawa Electric Corporation.

[Ed:05/b]

Printed in Japan, 807(KP)